

Temtop

M2000C

Model: M2000C

Elitech Technology, Inc.

1551 McCarthy Blvd, Suite 112,

Milpitas, CA 95035 USA

(+1)408-844-4070

sales@temtopus.com

www.temtopus.com

Made in China

Manual for Air Quality Detector

Product Overview

The hand-held air quality detector is a device which can test the concentration of carbon dioxide and numbers of particles in the air. It adopts a laser particle sensor and a carbon dioxide sensor based on NDIR detection theory and can transform the concentration of air pollutants to visual data directly, providing early air quality warning for you and protecting the health of your family effectively.

Application Scope

Indoors, Outdoors, Vehicles, etc.

Product Appearance



- Note: When the system enters the recording curve display interface, the data is updated every 2s under the abscissa 0-96s;
When the abscissa is 0-48min, the data is updated every 1min;
When the abscissa is 0-4h, the data is updated every 5min;
When the abscissa is 0-24h, the data is updated every 30min.

Product Specifications

- Name: Hand-held air quality detector
- Model: M2000C
- Display: color TFT LCD screen
- Battery voltage: 3.7VDC
- Overall dimension: 73.5*139*37.5 mm
- Power adapter:
 - Output voltage: DC5V
 - Output current: 1A
- Operating environment:
 - Temperature range: 0~50°C (32~122°F)
 - Humidity range: 0~90% RH
 - Atmospheric pressure: 1atm
- PM2.5 technical specification
 - Measurement range: 0-999ug/m³
 - Resolution: 0.1ug/m³
- PM10 technical specification
 - Measurement range: 0-999ug/m³
 - Resolution: 0.1ug/m³
- CO₂ technical specification
 - Measurement range: 0-5000PPM
 - Resolution: 1PPM

Air Quality Parameter for Reference

Status Pollutant	Good	Moderate	Unhealthy for Sensitive Groups	Unhealthy	Very Unhealthy	Hazardous
PM2.5 (μg/m ³)	≤12	12.1~35.4	35.5~55.4	55.5~150.4	150.5~250.4	≥250.5
PM10 (μg/m ³)	≤54	55~154	155~254	255~354	355~424	≥425
CO2 (ppm)	≤700	701~1000	1001~1500	1501~2500	2501~5000	≥5001


- ① Buzzer status: "🔊" indicates the buzzer is on. When measured pollutant concentration exceeds the upper alarm limit, the buzzer beeps. "🔇" indicates the buzzer is off. When an alarm is triggered, the buzzer will not beep.
- ② Display the two states of the detector: Paused or Runing. "Runing" indicates data is being detected. "Paused" indicates measurement pauses.
- ③ Date and time: Current date and time is displayed.
- ④ Battery power: Display the remaining battery power and the charging status of the detector.
 🔋: Battery is empty, please charge. 🔋: Battery is full. 🔋: Charging.
- ⑤ Main display area: Display measured data, curve, menu options.
- ⑥ Menu button: Press to pop up the menu options or shift the cursor position.
- ⑦ Up button: Press to increase setting values or shift up to select menu option.
- ⑧ Return button: Press to close current pop menu or return to the previous interface.
- ⑨ Power on/off or confirm: Press $\frac{OK}{\downarrow}$ for 2 seconds to turn on/off the instrument. It can also be used to confirm certain operation.
- ⑩ Down or run/pause button: Press to decrease setting values or move down to select menu option. It can also be used to continue or suspend detection on the detection interface.

Operation Notice

- Please keep the detector away from substances like fluff and hair to guarantee the accuracy of measured data.
- Please do not put the detector in the environment where the concentration of particles is more than 500ug/m³ and that of CO₂ is over 2500PPM for long time. Long-time exposure to high-concentration air pollutants will damage the sensor and make it work improperly.
- Avoid using the detector in humid environment to make sure the accuracy of test data.
- The product is a precision measurement instrument, so please do not bump, strike or drop the detector.
- Please do not cover the detection port or air outlet during use.


Operation Method

(1): Main menu interface

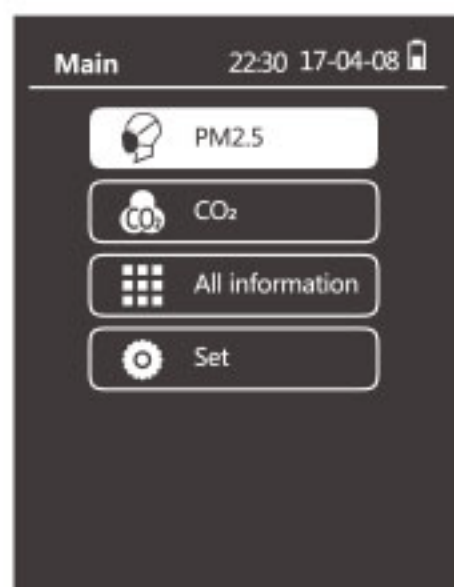


After the detector is turned on, it will enter the main menu interface automatically, displaying the following 4 options:

- ① PM2.5
- ② CO₂
- ③ All information
- ④ Set

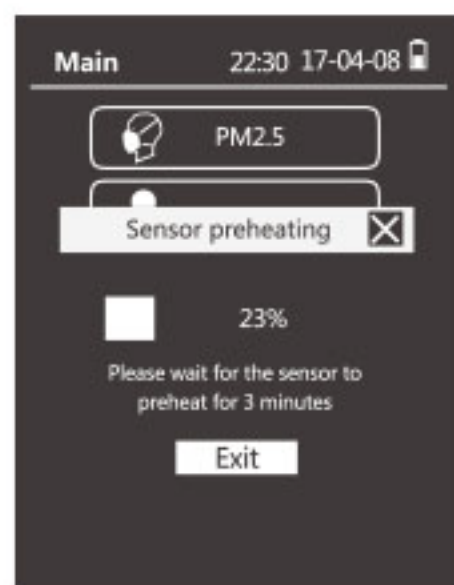


Press or key to choose an option and then press key to enter the interface. Before entering CO₂ concentration detection interface, the detector will have a pop-up window showing "sensor being preheated" if it is turned on for less than 3 minutes. The interface can be entered only after the sensor's preheating is finished.

(2): Interface of particles' concentration detection

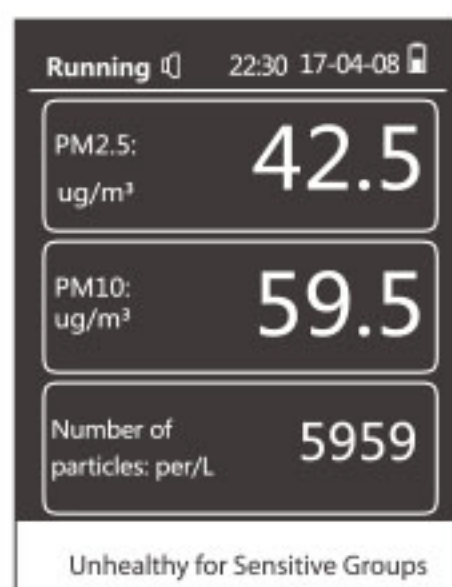

After switching from the main menu to particles' detection interface, the detector will show the real-time concentration of PM2.5, PM10 and particles as well as the level of pollution concentration;
If the value is beyond the set concentration's upper limit, the buzzer will give out the alarm;

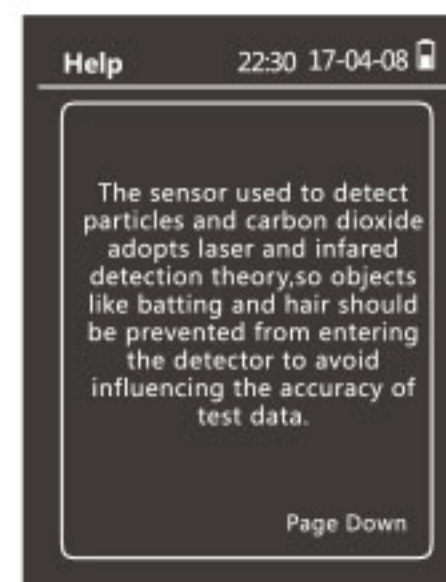

- ③ "Help": Press to enter the interface and then press or to view instructions and notices, then press to back to the interface of settings.




- ④ "Restore": Press key and then a window showing "Restore factory settings as default" will pop up. Press key to switch to "Restore" or "Not restore" key, and then you can press key to choose to restore or not restore factory settings as default and then return to the interface of setting. Factory default settings include: the upper-limit alarm value of various concentration and languages.




- ⑤ "Language": Select "Language" and press to enter this interface and then press to shift. Press to confirm the language option. Use to shift between "Save" or "Don't Save". Press and return to the interface of settings.

(5): Interface setting

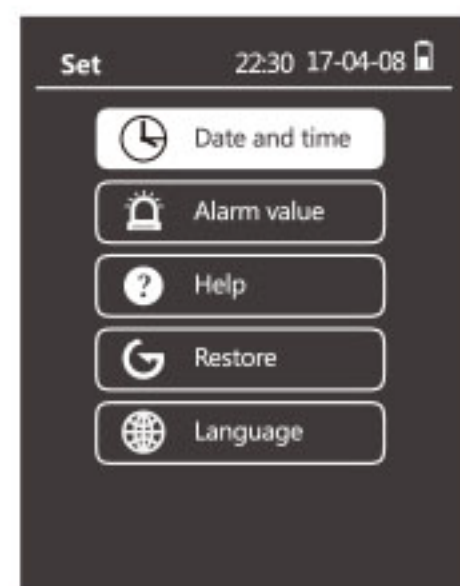


After switching from the main menu to the setting interface, the user will find the following 5 options shown on the screen. Press ▲ or ▼ key to choose the option you want to enter. Then Press $\frac{OK}{\downarrow}$ key to enter the corresponding interface or press $\frac{OK}{\uparrow}$ key to return to the main menu interface.

- ① "Date and time"
- ② "Alarm value"
- ③ "Help"
- ④ "Restore"
- ⑤ "Language"

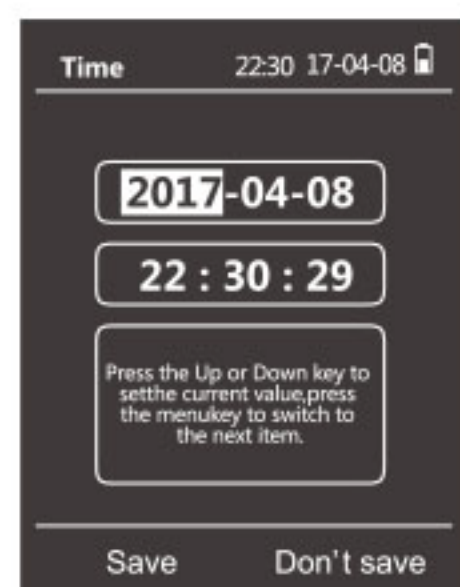


The functions of above menu items are as follows:

① "Date and time": In settings interface, select this option and press $\frac{OK}{\downarrow}$ to enter the interface and then press ▲ or ▼ to set the date. Press $\frac{OK}{\uparrow}$ to shift. After switching to "Save" or "Don't Save", press $\frac{OK}{\downarrow}$ to confirm the settings and back to the interface of settings.

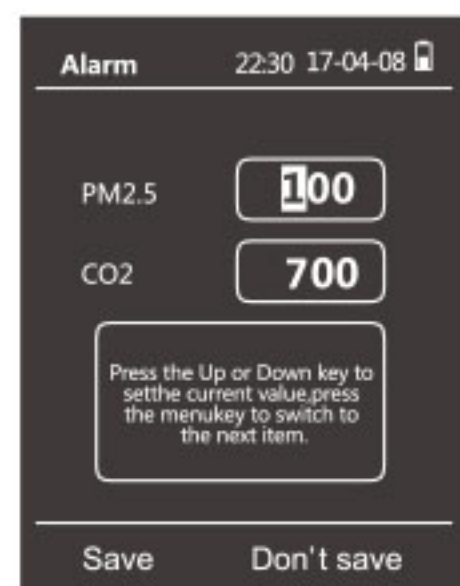


② "Alarm value": In settings interface, select this option and press $\frac{OK}{\downarrow}$ to enter the interface and then press ▲ or ▼ to set the upper-limit alarm value of PM2.5 or CO2 concentration. Press $\frac{OK}{\uparrow}$ to shift. After switching to "Save" or "Don't Save", press $\frac{OK}{\downarrow}$ to confirm the settings and back to the interface of settings.

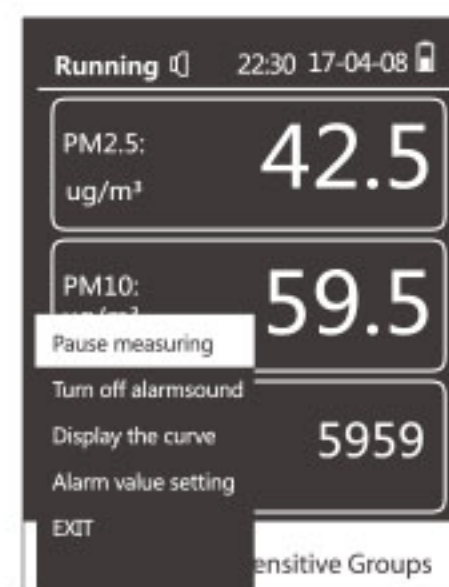


Press $\frac{OK}{\downarrow}$ key if you intend to pause or begin the detection;
Press $\frac{OK}{\uparrow}$ key if you intend to return to the interface of main menu;
Press $\frac{OK}{\uparrow}$ key, and then the following 5 options will be presented.
Press $\frac{OK}{\downarrow}$ key to enter into the corresponding function;

- ① "Pause or start measuring"
- ② "Turn on or off the alarm sound"
- ③ "Display or not display the curve"
- ④ "Alarm value setting"
- ⑤ "EXIT"

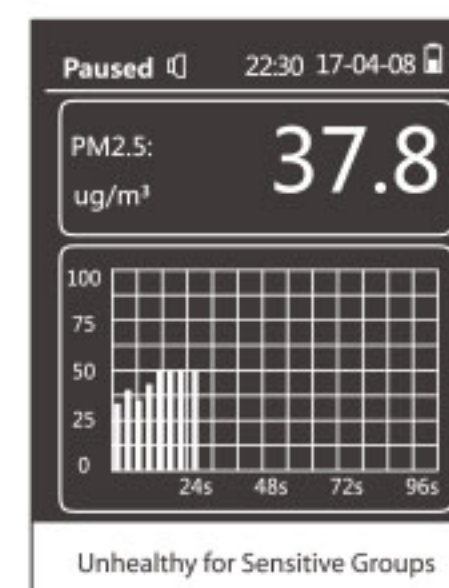


The functions of above menu items are described as below:

① "Pause or start measuring": Make the detector pause or start measuring the concentration of PM2.5, PM10 and particles as well as the level of pollution concentration.
② "Turn on or off the alarm sound": When the detected concentration is higher than the pre-set value, the buzzer will give out the alarm. Pressing this key can turn off or on the alarm function.
③ "Display or not display the curve": If you choose "Display the curve" function, the PM2.5 concentration curve will be shown in a visualized way. If you choose "Not display the curve" function, the curve display will be turned off.

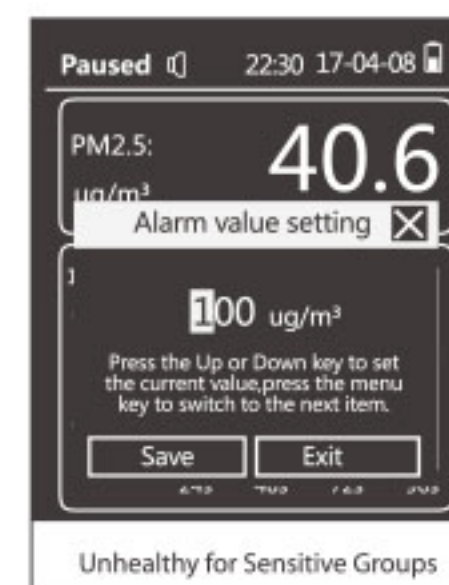


④ "Alarm value setting":
A window showing "Alarm value setting" will be popped up to remind you to set the upper-limit alarm value of PM2.5 concentration. Press $\frac{OK}{\uparrow}$ key to switch to the next item. Press ▲ or ▼ key to set the upper-limit alarm value. When $\frac{OK}{\uparrow}$ key is switched to "Save" or "Exit" key, you can press $\frac{OK}{\downarrow}$ key to choose to save or not save the set upper-limit alarm value of concentration and then close the pop-up window.
⑤ "Exit": Exit from the menu item and then return to the interface of detecting the concentration of particles.

(3): Interface of CO2 concentration detection

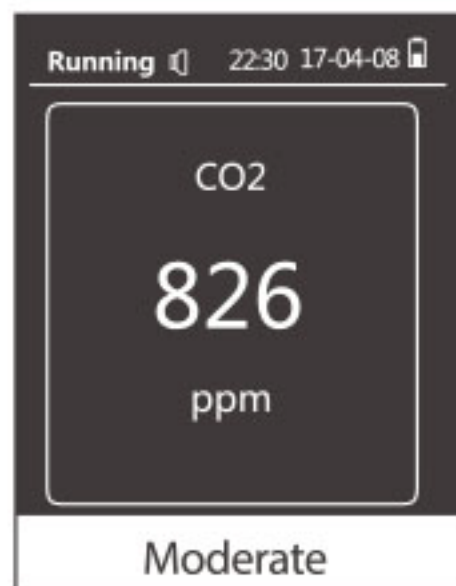

After switching from the main menu to CO2 detection interface, the detector will show the real-time concentration of CO2 and the "out of specification" status of pollution concentration; if the value is beyond the set concentration's upper limit value, the buzzer will give out the alarm;

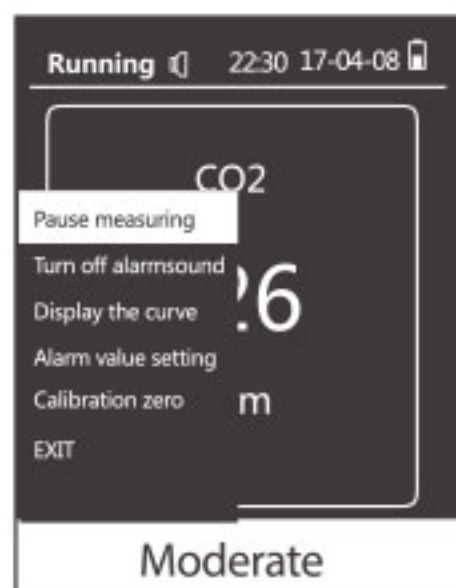


Press \blacktriangledown key if you intend to pause or begin the detection;
Press \blacksquare key if you intend to return to the interface of main menu;
Press \equiv key, and then the following 5 options will be presented.
Press $\frac{OK}{\downarrow}$ key to enter into the corresponding function;

- ① "Pause or start measuring"
- ② "Turn on or off the alarm sound"
- ③ "Display or not display the curve"
- ④ "Alarm value setting"
- ⑤ "Calibration zero"
- ⑥ "EXIT"

The functions of above menu items are described as below :

- ① "Pause or start measuring": Make the detector pause or start measuring the concentration of CO2 and the "out of specification" status of pollution concentration.
- ② "Turn on or off the alarm sound": When the detected concentration is higher than the pre-set value, the buzzer will give out the alarm. Pressing this key can turn off or on the alarm function.
- ③ "Display or not display the curve": If you choose "Display the curve" function, the CO2 concentration curve will be shown in a visualized way. If you choose "Not display the curve" function, the curve display will be turned off.

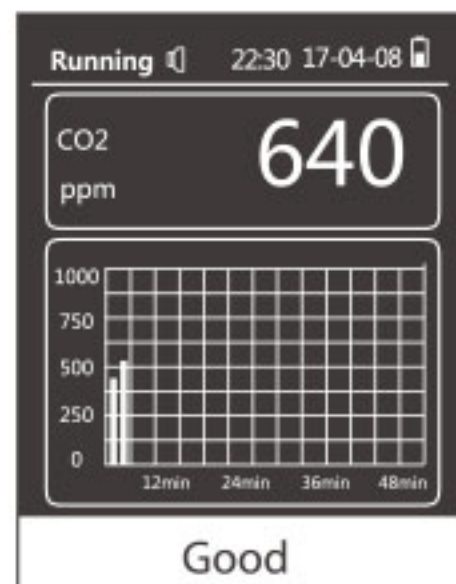


- ④ "Alarm value setting" Press \blacktriangle or \blacktriangledown to select this option and then press $\frac{OK}{\downarrow}$ to enter the interface. Press \blacktriangle or \blacktriangledown to adjust the upper-limit alarm value of CO2 concentration. Press \equiv to shift. After switching to "Save" or "Exit", press $\frac{OK}{\downarrow}$ to confirm the settings and back to the interface of settings.



- ⑤ "Calibration zero": The window showing "sensor under calibration" will be popped up for 30 minutes to calibrate the Zero point of CO2 sensor. You can exit calibration by pressing \blacksquare or $\frac{OK}{\downarrow}$ key.
- ⑥ "Exit": Exit from the menu item and then return to the interface of detecting the concentration of CO2.

(4): Interface of checking all information

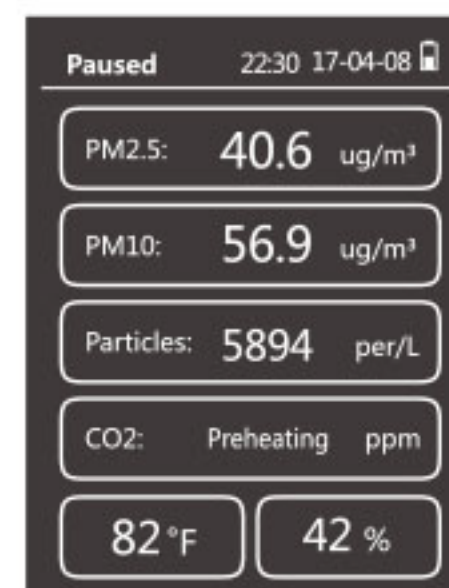

After switching from the main menu to the interface of checking all information, the user will see the concentration of PM2.5, PM10, particles and CO2 as well as the temperature and humidity shown on the detector.

- Press \equiv to switch between °C or °F.
Press \blacktriangledown key if you intend to pause or start measuring the concentration of PM2.5, PM10, particles and CO2.
Press \blacksquare key if you intend to return to the interface of main menu;